

DT 122 STAINLESS STEEL DIAPHRAGM SEAL

FEATURES

The DT122 diaphragm seal is designed for equipping pressure gauges, pressure transmitters and pressure switches which cannot be directly mounted in contact with a corrosive, viscous or crystallising liquid they measure the pressure of. The DT122 model with PN16 flange connection is removable and thus easy to service.

LIMITS OF USE


Fluid WP:	40 bar
Fluid WT° (outside filling liquid):	-40°C / +150°C

connection		Ø membrane (mm)	minimum range (bar)	maximum range (bar)
pressure gauge	process			
G 1/4" F	DN 15	36	0-10	0-40
G 1/2" F	DN 15	36	0/10	0-40
G 1/2" F	DN 20	45	0/6	0-40
G 1/2" F	DN 25	45	0/6	0-40




CONSTRUCTION

No.	Name	Material
a	Upper body	AISI 316 SS
b	Lower body	
c	Membrane	AISI 316 L stainless steel
d	Instrument fitting	n.a.
e	Filling orifice	n.a.
f	Process fitting	n.a.

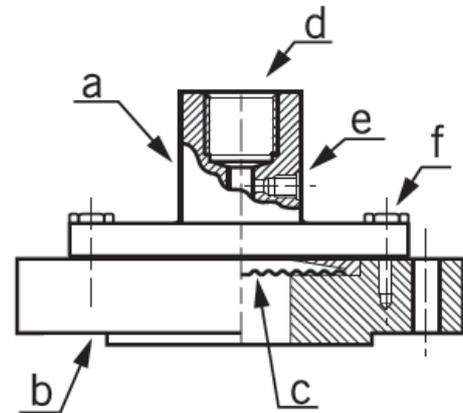

DIMENSIONS (mm) AND CONNECTIONS

	Membrane size		
	Ø	36	45
D1	95	105	115
T	16	18	
Bolt	Flat wrench		

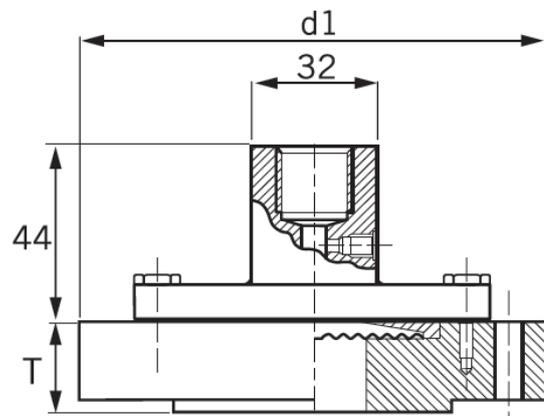

Information given as an indication only, and subject to possible modifications

DT 122 STAINLESS STEEL DIAPHRAGM SEAL

HOW TO CHOOSE A DIAPHRAGM SEAL


1. The diaphragm seal has to be chosen depending upon the process conditions (type of fluid, pressure, temperature, etc.) and upon the volume of the measuring device to protect.
2. The filling liquid has to be chosen depending upon the process conditions (type of fluid, pressure, temperature, etc.), upon the material of the measuring device to protect, and upon the type of application (standard or food-related).
3. The liquid used must not contain gas.

FILLING INSTRUCTIONS

1. Mount the pressure gauge onto the diaphragm seal using a suitable gasket to prevent leakage.
2. Bring the system chamber to vacuum by using the filling orifice reference mark (e).
3. Fill the chamber with the filling liquid chosen.
4. To provide optimum filling, push with compressed air (maximum 0.5 bar).
5. During the filling phase, it is important to balance the pressure on each side of the membrane to prevent its deformation.
6. Close the filling orifice (e).
7. Check that the liquid is not under pressure. If this is the case, release a little bit of pressure by losing the filling screw.
8. Check the membrane flatness.

INSTRUCTIONS FOR INSTALLING THE SYSTEM

1. Connect the diaphragm seal pressure gauge system to the process. To tighten the flange model, use a flat wrench and tighten the bolts. Use a gasket to prevent leakage between the diaphragm seal gasket connection and the process.
2. Diaphragm seals do not need servicing.
3. The diaphragm seal must not leak. If a leakage occurs, the pressure measurement will be wrong.
4. Pressure gauges lose one class of accuracy when mounted on a diaphragm seal.

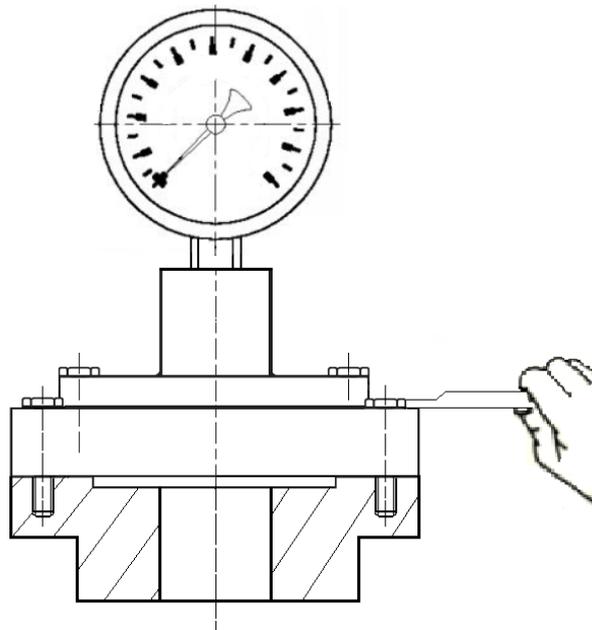

Information given as an indication only, and subject to possible modifications